

Micro-QuEChERS extraction coupled to GC–MS for a fast determination of Bisphenol A in human urine

Luísa Correia-Sá^{a,b}, Sónia Norberto^b, Cristina Delerue-Matos^a, Conceição Calhau^{b,c},
Valentina F. Domingues^{a,*}

^a REQUIMTE/LAQV-GRAQ, Instituto Superior de Engenharia, Instituto Politécnico do Porto, Rua Dr. António Bernardino de Almeida, 431, 4200-072 Porto, Portugal

^b CINTESIS – Center for Research in Health Technologies and Information Systems, Porto, Portugal

^c Nutrition & Metabolism, NOVA Medical School, Faculdade de Ciências Médicas, Universidade NOVA de Lisboa, Lisboa, Portugal

ABSTRACT

Bisphenol A (BPA) is considered an endocrine disruptor and public concern over BPA exposure has been raised. Several studies have assessed human exposure to this plasticizer, confirming its ubiquitous presence and highlighting children as a public of special concern. A simple, efficient, cheap and green analytical procedure is reported within this paper. This paper reports, for the first time, the development of a modified Micro-QuEChERS (Quick, Easy, Cheap, Effective, Rugged and Safe) method coupled to gas chromatography-mass spectrometry (GC–MS) as a new strategy for the efficient extraction and determination of Bisphenol A in human urine samples. Several parameters that are known to influence extraction were optimized. Good linearity was achieved at the studied concentration range (1–50 µg/L), with a correlation coefficient (R^2) of 0.998. The optimized method proved to be accurate ($\geq 74\%$ recovery), reproducible ($< 11\%$ relative standard deviation) and sensitive for BPA determination (detection limit of 0.13 µg/L and quantification limit of 0.43 µg/L). The analytical procedure was applied to the analyses of 12 urine samples collected from children living in the North/Center region of Portugal. BPA was detected in all the analyzed samples in concentrations ranging from 1.5 µg/L to 48.9 µg/L. The proposed methodology is suitable for the determination of BPA in urine samples in the framework of biomonitoring studies and bioanalytical analyses, applying GC–MS detection.

Keywords:

Bisphenol A

Micro-QuEChERS

Human urine

GC–MS

Children

1. Introduction

In the last decades, environmental exposure to certain industrial chemical substances has caused apprehension due to their potential toxicity and widespread use [1]. Bisphenol A (BPA), common name for 2,2-bis(4-hydroxyphenyl) propane is one of the major industrial chemicals of emerging concern [1].

Due to its cross-linking properties BPA has been widely used in the manufacture of polycarbonate plastics and epoxy resins, in the production of several products, such as food containers, food and beverage can linings, food packaging materials, CDs, medical equipment, bottles, plastic bags, etc [2]. Bisphenol A has been found to leach and migrate rather easily [2–13]. According to the available studies, BPA exposure from dietary sources is generally considered higher than exposure from non-food sources. Nevertheless, not all sources and routes of exposure contributing to the omnipresent BPA body burden are thoroughly understood [6,14,15].

BPA is considered an endocrine disruptor [2,5,16] and

consequently, public concern has been raised by several studies suggesting a link between BPA exposure with several health outcomes, namely obesity [17–25]. However, nowadays these human health effects from low-level exposures to BPA are being debated [4,16,26–32]. In 2015, the European Food and Safety Authority (EFSA) has lowered the Tolerable Daily Intake (TDI) for BPA to a temporary TDI (t-TDI) of 4 µg/kg body weight/day, based on new data and the uncertainties surrounding health effects in regard to mammary gland, reproductive, metabolic, neurobehavioral and immune systems [28]. Moreover, according to several studies, children seem to be a population of special concern as their exposure levels are higher when compared to adolescents and adults [33–35].

Pharmacokinetic studies showed that BPA is rapidly metabolized and conjugated predominantly with the glucuronic acid to the BPA-glucuronide in the gut wall and liver [36–41]. Since most of the BPA taken up orally is excreted in urine within less than 24 h, urine is the preferred matrix for estimating human exposure [38,42–44].

The identification and quantification of BPA is challenging, due to

* Corresponding author.

E-mail address: vfd@isep.ipp.pt (V.F. Domingues).

the low concentrations at which this compound is typically present in human matrices and due to a possible background contamination. Therefore, biomonitoring should be performed through highly sensitive analytical methods and exposure assessment based on the conjugates [45].

Common sample preparation techniques for BPA human biomonitoring methods include solid phase extraction (SPE) and liquid-liquid extraction (LLE) [5,46,47]. The demand of high-throughput methods in biomonitoring programs has led to the development of automated off-line and on-line SPE methods. These on-line SPE methods tend to reduce significantly the sample volume required and procedure time [48,49]. Generally, liquid chromatography coupled to mass spectrometry is the most common analytical technique for BPA determination, not requiring a derivatization step [38]. However, several studies have reported the use of gas chromatography with a prior derivatization step frequently associated with SPE as the extraction technique [5,38]. Additionally, some authors have addressed the comparison between GC and LC for the determination and quantification of a broad range of compounds, concluding that both techniques are comparable [50–52].

The QuEChERS (quick, effective, cheap, rugged and safe) methodology was initially developed in 2003 for the determination and measurement of pesticides residues in vegetables and fruits, combining the extraction/isolation of pesticides and extract clean-up [53]. This technique comprises extraction using commonly acetonitrile (ACN), as extraction solvent, and purifying the extract by dispersive solid-phase extraction (dSPE) [54]. Since then the QuEChERS technique has become the method of choice for food analysis and has suffered various modifications and improvements over the years. Therefore, nowadays this method is applied to other analytes and matrices [54,55].

This methodology has been applied for BPA determination in food matrices and animal organs, namely in seafood, canned food (seafood, vegetables and fruits), packed food, honey and rat testis [56–65]. In these studies, different compositions of QuEChERS salts were tested such as the original composition (NaCl and MgSO₄), citrate buffer (additional citrate buffers) and acetate buffer (additional acetate buffer). Nonetheless, the extraction solvent was always set to the ACN. The QuEChERS has also been used, in few occasions for the determination of pesticides [66–68], diverse environmental contaminants [46], pharmaceuticals [69,70] and lipids [71] in urine samples. For this matrix, different salt compositions were also tested and used, still ACN was once more the chosen extraction solvent, except for the lipids determination [71].

The present work displays a novel methodology based on QuEChERS technique coupled to GC–MS for BPA determination in human urine samples. As far as the authors know this is the first time this method has been applied with this aim. The developed method, based on miniaturized QuEChERS method presents several advantages when compared with more traditional extraction techniques (namely manually-operated SPE) as it is less laborious, time consuming, cheaper and greener (less solvent consumption). The present work is therefore relevant for human biomonitoring studies and biomedical analysis in GC–MS field.

2. Material and methods

2.1. Reagents and chemicals

GC-grade Hexane and Methanol, Acetonitrile (ACN) HPLC-grade (purity $\geq 99.9\%$) were purchased from Merck (Darmstadt, Germany). Commercially available bisphenol A (BPA, 2,2-(4,4-dihydroxydiphenyl) propane) (99% purity), and the isotope labeled internal standard ¹³C₁₂-BPA (99%) were provided by Sigma (St. Louis, MO, USA). The derivatization reagent was BSTFA + TMCS (99:1) (GC/GC–MS) from Supelco (Bellefonte, PA, USA). Three different types of QuEChERS and two dSPE were tested: QuEChERS A ((4 g magnesium sulfate (MgSO₄) and 1 g sodium chloride (NaCl)); QuEChERS B (6 g MgSO₄ and 1.5 g

anhydrous sodium acetate (CH₃COONa)); and QuEChERS C (6 g MgSO₄, 1.5 g NaCl, 1.5 g of sodium citrate dihydrate (Na₃Cit·2H₂O) and 0.750 g sodium citrate sesquihydrate (Na₂HCit·1.5H₂O)). The two tested dSPE had the following composition: dSPE 1) was composed of 25 mg of C18 ((octadecyl sorbent (C18)) and 150 mg of MgSO₄; and dSPE 2) was composed by 50 mg of primary and secondary amine (PSA) exchange material, 50 mg of C18 and 150 mg MgSO₄. The QuEChERS and the dSPE were supplied by Agilent technologies (Bond Elut Sample preparation solutions) (Lake Forest, CA, USA). For enzymatic hydrolysis was used the enzyme β -glucuronidase/arylsulfatase from *Helix pomatia* (EC 3.2.1.31/EC3.1.6.1; 5.5/2.6 U/mL) purchased from Roche Diagnostics (Indianapolis, USA).

2.2. Standard solutions

Stock solutions (100 mg/L) were prepared in methanol. Working solutions were prepared daily from these stocks by appropriate dilution. The solutions were stored at -20°C . Two five-concentration-level calibration curves within the 1–50 $\mu\text{g/L}$ concentration range in methanol and urine (matrix-matching calibration, spiked after extraction) were prepared. Deuterated internal standard (¹³C₁₂BPA) was employed to compensate for possible matrix effects and analyte losses.

2.3. Instrumentation

Chromatographic analysis was carried out in a TRACE GC Ultra gas chromatograph Polaris Q coupled with ion trap mass spectrometer (Thermo Fisher Scientific) operated in the electron impact ionization (EI) mode at 70 eV and controlled by Xcalibur 1.3. The helium carrier gas (Linde Sogas purity $\geq 99.999\%$) was maintained at a constant flow of 1 mL/min. Injection (2 μL) was carried in splitless mode. A Phenomenex column ZB-XLB (30 m x 0.25 mm I.D, 0.25 μm film thickness) was used. The GC oven temperature was programmed from an initial temperature of 90 $^{\circ}\text{C}$ (1 min hold), ramped at 15 $^{\circ}\text{C}/\text{min}$ up to 250 $^{\circ}\text{C}$ (1 min hold), increased to 255 $^{\circ}\text{C}$ at 20 $^{\circ}\text{C}/\text{min}$ (5 min hold) and finally to 270 $^{\circ}\text{C}$ at 10 $^{\circ}\text{C}/\text{min}$ (1 min hold). This program resulted in a total run time of 23.42 min. The other optimized parameters included a transfer line temperature of 250 $^{\circ}\text{C}$ and an ion source of 250 $^{\circ}\text{C}$. The BPA was quantified in the selected ion monitoring (SIM). The selected ions for BPA were 357 and 372, for ¹³C₁₂BPA were 364 and 383, and the retention time of the compounds was 12.85 min. The identification was confirmed by retention times and ion ratios. To homogenize the samples a VWR vortex mixer (Radnor, Delaware, USA) was used. For centrifugation, a Thermo Scientific™ Heraeus™ Megafuge™ 16 Centrifuge (Germany) was applied.

2.4. Urine samples

Urine samples were obtained from voluntary children that were normal and obese/overweight. The study was approved by the ethics committee of the Centro Hospitalar S. João/FMUP (Medicine Faculty of Oporto University ref. 163.13) and all the parents provided written consent. All samples were stored in glass material at -20°C until analysis. Urinary creatinine concentration was measured through a modified Jaffe method [72] with an Olympus AU5400® (Beckman-Coulter®, Porto, Portugal) at São João Hospital, Department of Clinical Pathology.

2.5. Micro-QuEChERS optimization

Different composition of QuEChERS (Original, AOAC and EN methods) salts as well as two dSPE (dSPE 1 and dSPE 2) were tested through preliminary recovery studies. Additionally, several parameters that can affect the extraction efficiency were analyzed. During method optimization, the following parameters were evaluated: urine (1.0 and 1.5 mL) and ACN (1.0, 1.5 and 3 mL) volumes; ACN acidification (1%

acetic acid); different masses of the selected QuEChERS (500 and 750 mg); ideal volume of the final extract (100, 200, 400 and 500 μ L) used prior to derivatization.

After optimization, the samples were analyzed according to the following procedure. An aliquot of 1.5 mL of homogenized urine was mixed into an 8 mL glass vial with 25 μ L of β -glucuronidase/aryl sulfatase enzyme (to hydrolyze glucuronide- or sulfate-conjugated metabolites), and the internal standard. The samples were incubated overnight at 37 $^{\circ}$ C. After the enzymatic hydrolysis took place, an optimized Micro-QuEChERS procedure was employed to extract BPA from urine samples. To the hydrolyzed sample were added 750 mg of QuEChERS B (AOAC method) and 3 mL of ACN. The mixture was strongly shaken in a vortex for 1 min and then centrifuged during 10 min at 4500 rpm. The obtained ACN layer was immediately transferred into the 2 mL dSPE 1, mixed for 1 min and centrifuged for 10 min at 4500 rpm. Later, 200 μ L of the extract were transferred to a GC vial and evaporated to dryness under a gentle stream of nitrogen. The dry residue was then dissolved in 100 μ L of derivatization reagent (BSTFA + 1% TMCS). This mixture was put in a bath at 80 $^{\circ}$ C for 30 min, following the derivatization conditions (time and temperature) previously reported by Kuo and Ding [73]. The final extract was transferred into a glass insert (into a GC Vial) and analyzed using the GC-MS system.

2.6. Method validation

The method was validated for linearity, detection and quantification limits (LOD and LOQ, respectively), selectivity, accuracy, recovery and precision, according to international guidelines [74–76].

The selectivity of the method was analyzed by comparing the chromatograms of several blank urine samples with those of the spiked (BPA) urine samples.

A five point matrix-matched calibration curve was obtained using human urine samples fortified, after extraction, with BPA at concentrations from 1 to 50 μ g/L (three replicates of each). The calibration curve was constructed using analyte/internal standard peak area ($^{13}\text{C}_{12}$ BPA) ratio versus concentration of the analyte in urine matrix. A calibration curve was also constructed with standard solutions in the same linear range for the evaluation of possible matrix effects. In this study, the LOD and LOQ were calculated with S/N 3 and 10 of the lowest analyzed concentration, respectively.

Generally, the term Accuracy refers to the trueness and precision of the method. Concerning trueness, several approaches can be applied. In the present study accuracy is expressed as recovery and was calculated through the spiking recovery method (%) [76]. Recovery studies were performed at spiking levels of 10, 20, 50 μ g/L. The mean peak areas of the urine samples spiked before and after extraction were compared. The interday precision and the intraday precision of the method were evaluated at two concentration levels, of 20 and 50 μ g/L. For the intraday precision, three replicates were analyzed on one day ($n = 3$), whereas for the interday precision, three replicates were analyzed on three consecutive days ($n = 9$). The results were expressed as the percent relative standard deviation (RSD).

3. Results and discussion

3.1. Modified QuEChERS optimization

During method optimization, background contamination was addressed, as exogenous sources of contamination are reported to be problematic when measuring this compound [77,78]. Glassware was used whenever possible and cleaned with hexane to eliminate any potential background contamination.

3.1.1. Micro-QuEChERS and dispersive SPE content

In the initial optimization tests a urine volume of 1 mL was used as other authors [67,71] reported good recoveries using similar amounts

of sample. Additionally, the original method (10 g or mL sample per 10 mL of extraction solvent) was scaled by using 1 mL of urine, 500 mg from each tested QuEChERS content (weighed into a glass flask) and 1 mL of ACN. The extraction solvent was set to ACN as this solvent is known to be more efficient than others, such as acetone and methanol [53,79]. Moreover, ACN has been used successfully in the extraction of several compounds [46,66–70] from urine matrix.

As described in Section 2.1 (from material and methods), in the present study three different QuEChERS (A, B and C) and two dSPE (1 and 2) compositions were tested. In a preliminary test, to select the best possible composition and combination, the obtained peak areas from urine samples fortified before extraction were compared with the peak area of a standard solution, all at concentration level of 50 μ g/L. Concerning the QuEChERS content, the AOAC composition (B) gave the best recoveries (from 92 to 120%). This composition was also successfully applied to the determination of disulfoton and its oxidative metabolites in human whole blood and urine samples (recoveries ranging from 87 to 112%) [67].

For the clean-up step, the dSPE 1, constantly, presented higher recoveries ($\geq 100\%$) than the dSPE 2 (from 69 to 92%), when combined with all the tested QuEChERS. Therefore, dSPE 1 composed of 25 mg of C18 and 150 mg of MgSO_4 was selected.

In a second approach to perform a more precise recovery experiment, accounting for the matrix effects, only the combination of the QuEChERS A, B and C with the dSPE 1 was evaluated. For analyzing recoveries, the obtained extracts peak areas (spiked pre-extraction) were compared with the peak area of a spiked matrix extract (spiked post-extraction) also at concentration of 50 μ g/L (Fig. 1).

Finally, ACN, as extraction solvent, QuEChERS B with the AOAC salts (MgSO_4 , CH_3COONa) and the dSPE 1 (25 mg of C18 and 150 mg of MgSO_4) were selected for sample preparation, as this combination presented higher recoveries (102%) with good peak shapes and removal of matrix interferences.

3.1.2. Acidification of the extraction solvent

As pointed out previously the original QuEChERS composition has suffered modifications to improve the extraction of pH sensitive compounds and in addition to minimize their degradation [80,81]. According to the AOAC 2007.01 method, an acidification of the extraction solvent occurs (ACN with 1% of acetic acid) [80]. Consequently, the ACN acidification was tested and evaluated. We believe that is the first time an acidification of the ACN was also tested for the EN 15562 method and the Original composition for urine samples. A signal

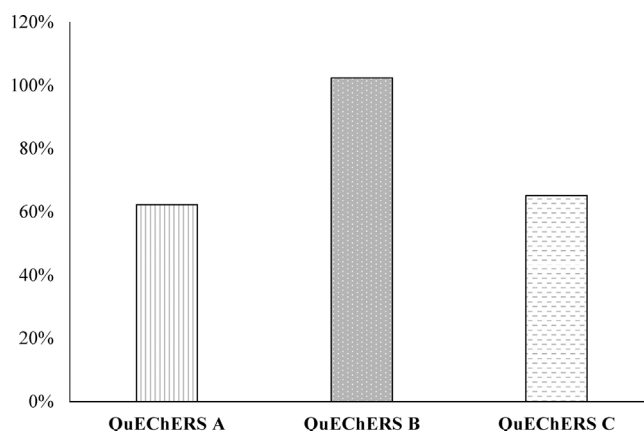


Fig. 1. Recoveries obtained with the three composition of QuEChERS salts combined with dSPE 1 clean-up (comparison between a matrix sample spiked before and after extraction at concentration level of 50 μ g/L) ($n = 1$). QuEChERS A (4 g magnesium sulfate (MgSO_4) and 1 g sodium chloride (NaCl)); QuEChERS B (6 g MgSO_4 and 1.5 g anhydrous sodium acetate (CH_3COONa)); and QuEChERS C (6 g MgSO_4 , 1.5 g NaCl , 1.5 g of sodium citrate dihydrate ($\text{Na}_3\text{Cit} \cdot 2\text{H}_2\text{O}$) and 0.750 g sodium citrate sesquihydrate ($\text{Na}_2\text{HCit} \cdot 1.5\text{H}_2\text{O}$)).

Table 1

Recoveries obtained during the experiments with the modified micro AOAC 2007.01 (ACN without acidification) QuEChERS method.

Experiments	Urine (mL)	QuEChERS B (mg)	ACN (mL)	Recoveries (%)
A	1.0	500	1.0	102
B	1.5	500	1.0	73
C		750	1.5	119
D		750	3.0	107

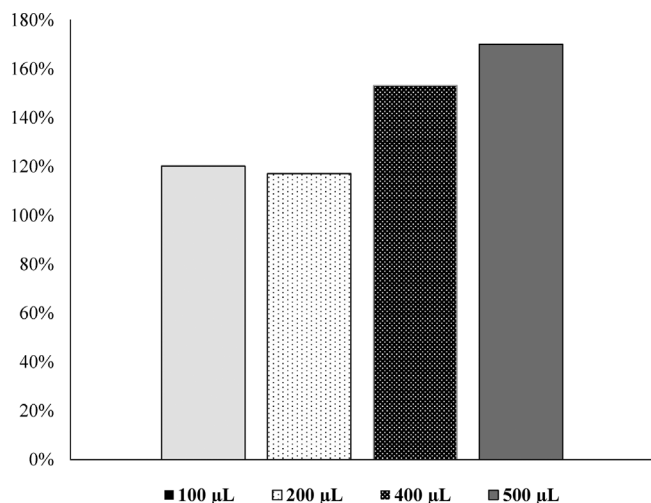


Fig. 2. Obtained matrix effects with the different extract volumes (matrix sample spiked before extraction compared with a standard at concentration level of 50 µg/L) (n = 1).

enhancement for these experiments could not be avoided, probably due to the presence of acetic acid as referred by other authors [82]. Furthermore, the chromatogram with AOAC salt composition and extraction with ACN without acidification, besides giving a good recovery (102%) also shown less matrix interferences. Therefore, the AOAC salt composition combined with the non-acidified ACN was chosen for further optimization studies.

3.1.3. Ratio of mass of QuEChERS content per volume of solvent and sample

After the QuEChERS and dSPE selection, different amounts of the selected QuEChERS and different ACN and urine volumes were tested in four experiments. The results of these tests are depicted in Table 1.

Overall, good recoveries were obtained with all the tested experiments. However, experiment D was chosen since it better separated the organic phase from the aqueous which allowed an easier removal of 2 mL to the clean-up (dSPE).

3.1.4. Selection of the volume of matrix extract

Optimizing the method further, the ideal volume of extract (removed after the dSPE), to be employed in the derivatization, was evaluated. Four extract volumes (according to experiment D), namely 100, 200, 400 and 500 µL were tested. After derivatization, the peak areas obtained from the analyzed extracts were divided by the peak area of a standard, all at concentration level of 50 µg/L. In Fig. 2 the observed matrix effects are shown.

The extract volume of 200 µL was selected as it showed a lower matrix effect (+10%) compared to other tested volumes. A possible explanation is that by concentrating more the presence of matrix components increased leading to higher matrix effects. For the volumes of 400 and 500 µL, dried and re-dissolved in 100 µL of the derivatization reagent (concentration factor of 4 and 5) the observed matrix effects were of +50 and +70%, respectively. The optimized procedure is shown in Fig. 3.

3.2. Method validation

A complete method validation, comprising linearity, selectivity, sensitivity, accuracy, precision (within day) and ruggedness (between days), was performed. In addition, matrix effects were also studied.

At BPA retention time, no interferences from endogenous substances were detected. Consequently, a good separation was obtained under the described GC-MS conditions. A chromatogram of a urine sample spiked with 50 µg/L of BPA is depicted in Fig. 4.

The capacity to quantify levels of target analytes in biological samples accurately and precisely involves the use of highly sensitive and selective instrumentation, namely through tandem mass

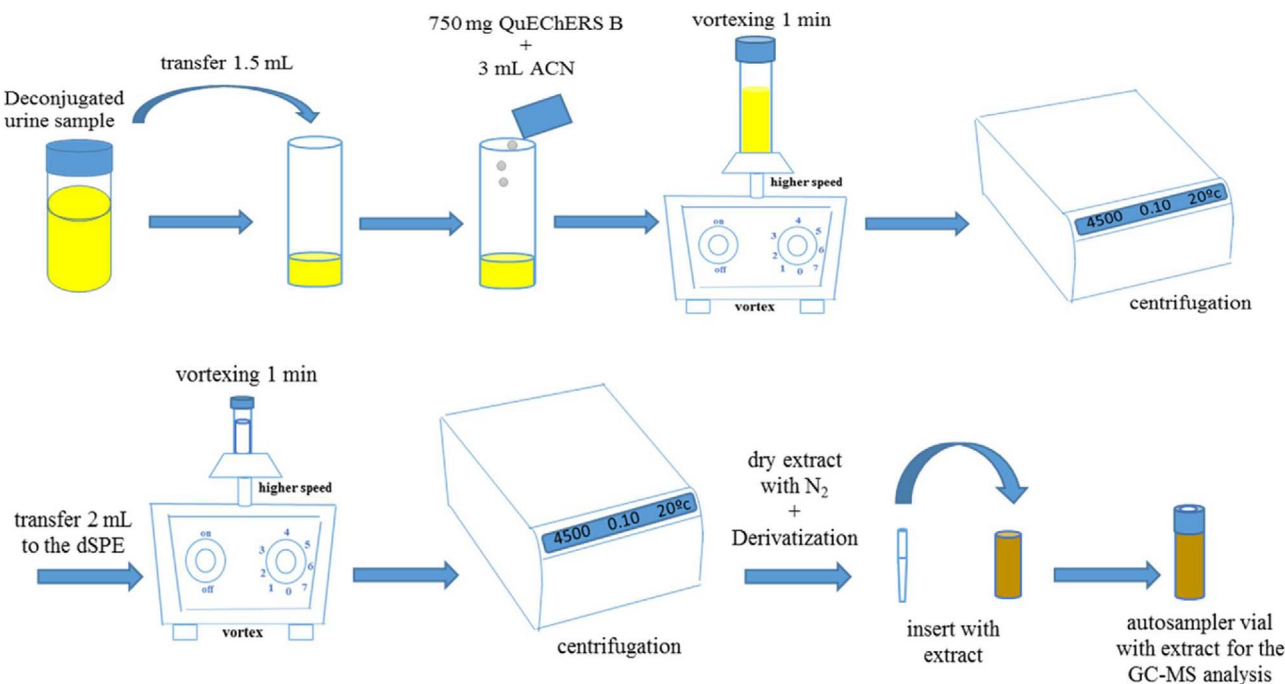


Fig. 3. Scheme of the optimized Micro-QuEChERS extraction for BPA analysis in urine.

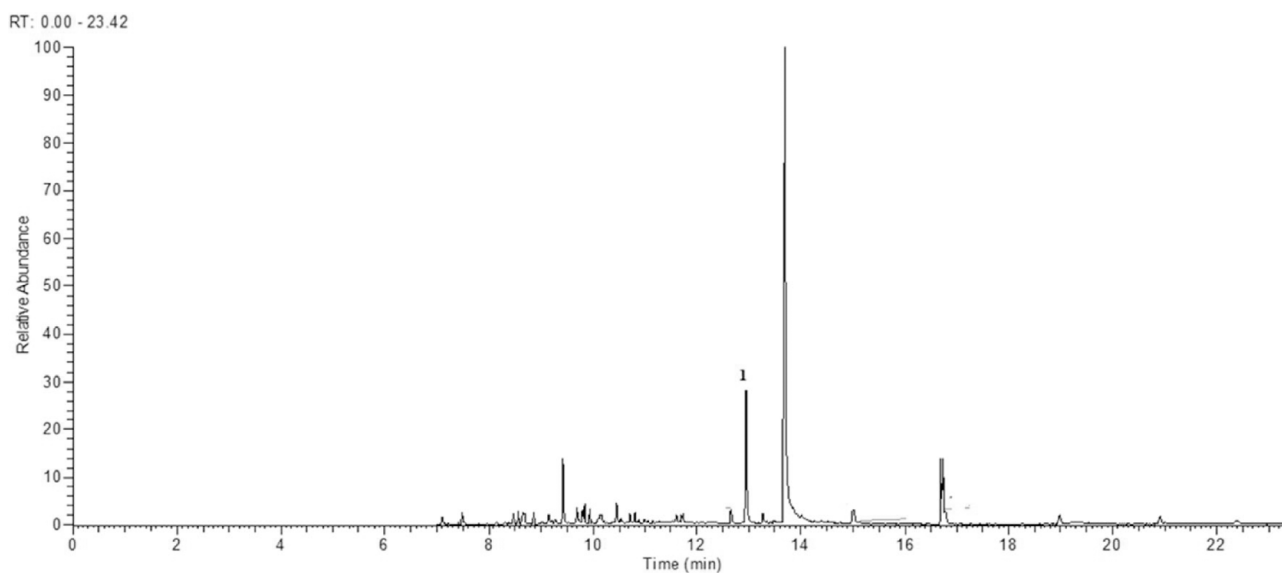


Fig. 4. Gas chromatography–tandem mass spectrometry separation profile of Bisphenol A at a spiking level of 50 µg/L in human urine (1-Bisphenol A).

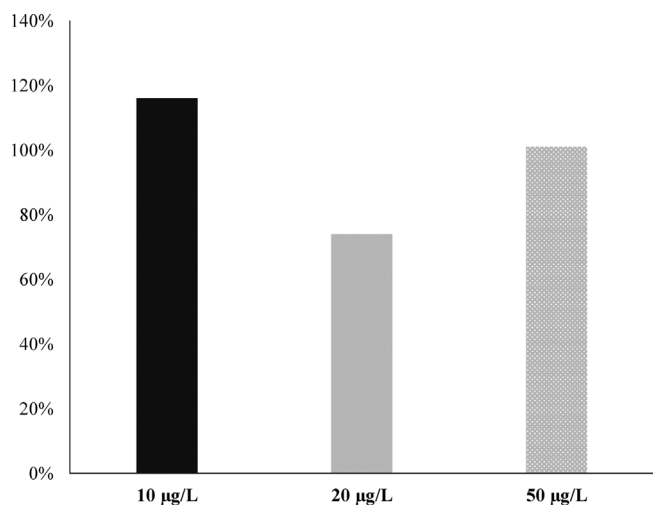


Fig. 5. BPA recoveries percentages from three spiked urine samples at concentration level of 10, 20 and 50 µg/L.

spectrometry and a comprehensive understanding of extremely variable matrix effects. Usually, matrix effects are caused by the co-elution of matrix components that modify the ionization as well as the chromatographic response of target analytes, leading to reduced or increased sensitivity of the analysis. Therefore, before accuracy and precision are evaluated, these effects should be characterized and controlled. The

term, “matrix effects,” was first discussed by Tang and Kebarle [83] and it generally refers to a difference in mass spectrometric response for an analyte in standard solution versus the response for the same analyte in matrix [83].

Several approaches can be applied to determine the matrix effect in biological samples such as flow-based evaluation, post-extraction spike matrix comparison, and some alternative methods such as adding known amounts of target compounds to biological matrices obtained from at least ten donors [84].

Each biological matrix has a unique composition, urine is a complex sample with a general composition that includes salts, organic molecules (e.g., urea and amino acids), proteins (e.g., albumin and immunoglobulins), crystals (e.g., calcium phosphate and uric acid) and cells (white blood cells and transitional cells) [85]. Additionally, according to the diet and hydration status of the donors the amount of the matrix components can change [85].

To evaluate the matrix effect, the slopes obtained in the calibration with matrix matched-standards (spiked after extraction) were compared with those obtained with standard solutions according to other reports [84,86]. In general, a signal enhancement was observed (+ 44%).

Common strategies can be used to minimize or compensate for matrix effects in GC–MS method. A combination of these approaches is recommended to successfully manage matrix effects so that they will not alter method accuracy and precision [84]. Therefore, matrix-matched calibration was used for quantification purposes and additionally we used an isotopically labeled analogue of the target analyte as an

Table 2
Total BPA obtained in children's' urine (µg/L and µg/g creatinine).

Sample	Gender	Age	Weight group	Creatinine (g/L)	Total BPA (µg/L)	Total BPA (µg/g creatinine)
1	M	7	Obese/overweight	0.90	15.9	17.67
2	F	14	Obese/overweight	1.09	7.9	7.25
3	F	15	Obese/overweight	2.28	7.5	3.29
4	M	12	Normal	2.43	19.0	7.82
5	M	16	Normal	2.58	48.9	18.95
6	M	4	Normal	0.83	9.1	10.96
7	F	8	Obese/overweight	0.28	5.8	20.71
8	F	6	Obese/overweight	0.86	4.9	5.70
9	M	10	Obese/overweight	0.73	2.5	3.42
10	M	9	Obese/overweight	1.05	1.7	1.62
11	M	8	Obese/overweight	1.33	3.0	2.26
12	F	10	Obese/overweight	0.57	1.5	2.63

internal standard. This last approach is considered one of the most effective ways to rectify or account for matrix effects [86]. We obtained a linear response, over the concentration range from 1 to 50 µg/L, a slope of 0.0048 µg/L, with a correlation coefficient of 0.998. The obtained LOD and LOQ were of 0.13 and 0.43 µg/L, respectively. The methods LOD and LOQ were in the same range [87] (limit of detection of 0.1 ng/mL, applying UPLC-MS/MS) or even lower [88] (lower limit of quantification of 50 ng/mL, applying GC-MS) than other recently reported methods for BPA determination in urine samples.

The mean recoveries ($n = 3$ for each spiking level) and RSD for BPA, obtained with urine samples spiked at 10, 20 and 50 µg/L, measured by GC-MS (SIM mode), are shown in Fig. 5. Overall, good recoveries (from 70 to 120%) were obtained, and the percent relative standard deviations for recovery at different spiking levels ranged from 3 to 11%. The intraday precision and the interday precision of the method ranged from 3% to 10% and from 4% to 9%, respectively. Therefore, the developed method can be regarded as useful and appropriated for the quantification of BPA in urine samples.

3.3. Application to urine samples

The developed and optimized method was applied for the determination of total BPA in 12 randomly selected children, including both male and female subjects, with normal weight and obese/overweight. The samples were collected in 2014/2016. The age range was from 4 to 16 years old, with an average of 10 years old. The results obtained with the human urine samples are summarized in Table 2. The results showed that total BPA was detected in all the participant subjects at various degrees of concentrations, ranging from the lowest level at 1.5 µg/L to the highest at 48.9 µg/L. Values for total BPA were adjusted to the total creatinine content in the urine sample (Table 2).

4. Conclusions

With this study, for the first time, a new sample preparation method based on a miniaturized QuEChERS for BPA determination in human urine samples was presented. The optimized Micro-QuEChERS coupled to GC-MS, with derivatization, can be regarded as a sensitive and specific method for the quantification of total BPA in urine samples. Excellent recoveries were obtained, calibration was linear up to 50 µg/L with a LOQ of 0.43 and LOD of 0.13 µg/L, respectively. Traditionally GC-MS based methods (namely applying manually-operated SPE) for BPA determination in urine sample are laborious, time consuming and include numerous steps that can lead to background contamination. The proposed method is quick (can be performed in less than 1 h), easy, cheap and rugged. Additionally, it can be regarded as a greener alternative to traditional methods requiring smaller sample and extraction solvent volumes. The QuEChERS technique proved once more its versatility and may be a possible value tool for the biomedical analysis and biomonitoring studies in GC-MS field.

Conflict of interest statement

The authors declared no conflict of interest.

Funding sources

Lúisa Correia-Sá is grateful to FCT by the grant (SFRH/BD/87019/2012), financed by POCH, subsidized by Fundo Social Europeu and Ministério da Ciência, Tecnologia e Ensino Superior.

The authors are thankful to the project Qualidade e Segurança Alimentar – uma abordagem (nano) tecnológica, reference NORTE-01-0145-FEDER-000011.

References

- [1] M. Casas, C. Chevrier, E.D. Hond, M.F. Fernandez, F. Pierik, C. Philippat, R. Slama, G. Toft, S. Vandentorren, M. Wilhelm, M. Vrijheid, Exposure to brominated flame retardants, perfluorinated compounds, phthalates and phenols in European birth cohorts: ENRIECO evaluation, first human biomonitoring results, and recommendations, *Int. J. Hyg. Environ. Health* 216 (2013) 230–242, <http://dx.doi.org/10.1016/j.ijheh.2012.05.009>.
- [2] P. Fenichel, N. Chevalier, F. Brucker-Davis, A. Bisphenol, An endocrine and metabolic disruptor, *Ann. Endocrinol.* 74 (2013) 211–220, <http://dx.doi.org/10.1016/j.ando.2013.04.002>.
- [3] J.M. Braun, R. Hauser, Bisphenol A and children's health, *Curr. Opin. Pediatr.* 23 (2011) 233–239, <http://dx.doi.org/10.1097/MOP.0b013e3283445675>.
- [4] B.S. Rubin, A. Bisphenol, An endocrine disruptor with widespread exposure and multiple effects, *J. Steroid Biochem. Mol. Biol.* 127 (2011) 27–34, <http://dx.doi.org/10.1016/j.jsmb.2011.05.002>.
- [5] L. Correia-Sá, C. Calhau, C. Delerue-Matos, V.F. Domingues, Chapter 3: BPA evaluation in human samples, in: Y. Gibert (Ed.), *Bisphenol A: Sources, Risks of Environmental Exposure and Human Health Effects*, Nova Science Publishers, 2014, pp. 33–124.
- [6] T. Geens, D. Aerts, C. Berthot, J.-P. Bourguignon, L. Goeyens, P. Lecomte, G. Maghuin-Rogister, A.-M. Pironnet, L. Pussemier, M.-L. Scippo, J. Van Loco, A. Covaci, A review of dietary and non-dietary exposure to bisphenol-A, *Food Chem. Toxicol.* 50 (2012) 3725–3740, <http://dx.doi.org/10.1016/j.fct.2012.07.059>.
- [7] X.L. Cao, C. Perez-Locas, G. Dufresne, G. Clement, S. Popovic, F. Beraldin, R.W. Dabeka, M. Feeley, Concentrations of bisphenol A in the composite food samples from the 2008 Canadian total diet study in Quebec City and dietary intake estimates, *Food Addit. Contam. A* 28 (2011) 791–798, <http://dx.doi.org/10.1080/19440049.2010.513015>.
- [8] T. Geens, T.Z. Apfelbaum, L. Goeyens, H. Neels, A. Covaci, Intake of bisphenol A from canned beverages and foods on the Belgian market, *Food Addit. Contam. A* 27 (2010) 1627–1637, <http://dx.doi.org/10.1080/19440049.2010.508183>.
- [9] G.O. Noonan, L.K. Ackerman, T.H. Begley, Concentration of bisphenol A in highly consumed canned foods on the U.S. market, *J. Agric. Food Chem.* 59 (2011) 7178–7185, <http://dx.doi.org/10.1021/jf201076f>.
- [10] X. Li, G.-G. Ying, J.-L. Zhao, Z.-F. Chen, H.-J. Lai, H.-C. Su, 4-Nonylphenol, bisphenol-A and triclosan levels in human urine of children and students in China, and the effects of drinking these bottled materials on the levels, *Environ. Int.* 52 (2013) 81–86, <http://dx.doi.org/10.1016/j.envint.2011.03.026>.
- [11] R.S. Hehn, NHANES data support link between handling of thermal paper receipts and increased urinary bisphenol A excretion, *Environ. Sci. Technol.* 50 (2016) 397–404, <http://dx.doi.org/10.1021/acs.est.5b04059>.
- [12] T. Geens, L. Goeyens, K. Kannan, H. Neels, A. Covaci, Levels of bisphenol-A in thermal paper receipts from Belgium and estimation of human exposure, *Sci. Total Environ.* 435–436 (2012) 30–33, <http://dx.doi.org/10.1016/j.scitotenv.2012.07.001>.
- [13] Y. Lv, S. Lu, Y. Dai, C. Rui, Y. Wang, Y. Zhou, Y. Li, Q. Pang, R. Fan, Higher dermal exposure of cashiers to BPA and its association with DNA oxidative damage, *Environ. Int.* 98 (2017) 69–74, <http://dx.doi.org/10.1016/j.envint.2016.10.001>.
- [14] K.L.Y. Christensen, M. Lorber, S. Koslitz, T. Brüning, H.M. Koch, The contribution of diet to total bisphenol A body burden in humans: results of a 48 hour fasting study, *Environ. Int.* 50 (2012) 7–14, <http://dx.doi.org/10.1016/j.envint.2012.09.002>.
- [15] T. Geens, L. Goeyens, A. Covaci, Are potential sources for human exposure to bisphenol-A overlooked? *Int. J. Hyg. Environ. Health* 214 (2011) 339–347, <http://dx.doi.org/10.1016/j.ijheh.2011.04.005>.
- [16] J.G. Teeguarden, S. Hanson-Drury, A systematic review of Bisphenol A low dose studies in the context of human exposure: a case for establishing standards for reporting low-dose effects of chemicals, *Food Chem. Toxicol.* 62 (2013) 935–948, <http://dx.doi.org/10.1016/j.fct.2013.07.007>.
- [17] H.-x. Wang, Y. Zhou, C.-x. Tang, J.-g. Wu, Y. Chen, Q.-w. Jiang, Association between bisphenol A exposure and body mass index in Chinese school children: a cross-sectional study, *Environ. Health Perspect.* 11 (2012) 79, <http://dx.doi.org/10.1186/1476-069X-11-79>.
- [18] A. Shankar, S. Teppala, C. Sabanayagam, Urinary bisphenol A levels and measures of obesity: results from the national health and nutrition examination survey 2003–2008, *ISRN Endocrinol.* 2012 (2012) 1–6, <http://dx.doi.org/10.5402/2012/965243>.
- [19] L. Trasande, T.M. Attina, J. Blustein, Association between urinary Bisphenol A concentration and obesity prevalence in children and adolescents, *JAMA* 308 (2012) 1113–1121, <http://dx.doi.org/10.1001/2012.jama.11461>.
- [20] L.A. Hoepner, R.M. Whyatt, E.M. Widen, A. Hassoun, S.E. Oberfield, N.T. Mueller, D. Diaz, A.M. Calafat, F.P. Perera, A.G. Rundle, Bisphenol A and adiposity in an inner-city birth cohort, *Environ. Health Perspect.* 124 (2016) 1644–1650, <http://dx.doi.org/10.1289/ehp205>.
- [21] J.M. Braun, B.P. Lanphear, A.M. Calafat, S. Deria, J. Khoury, C.J. Howe, S.A. Venners, Early-life bisphenol A exposure and child body mass index: a prospective cohort study, *Environ. Health Perspect.* 122 (2014) 1239–1245, <http://dx.doi.org/10.1289/ehp.1408258>.
- [22] M. Hao, L. Ding, L. Xuan, T. Wang, M. Li, Z. Zhao, J. Lu, Y. Xu, Y. Chen, W. Wang, Y. Bi, M. Xu, G. Ning, Urinary bisphenol A concentration and risk of central obesity in Chinese adults: a prospective study, *J. Diabetes* (2017), <http://dx.doi.org/10.1111/1753-0407.12531>.
- [23] M. Vafeiadi, T. Roumeliotaki, A. Myridakis, G. Chalkiadaki, E. Fthenou, E. Dermizaki, M. Karachaliou, K. Sarri, M. Vassiliaki, E.G. Stephanou, M. Kogevinas,

- L. Chatzi, Association of early life exposure to bisphenol A with obesity and cardiometabolic traits in childhood, *Environ. Res.* 146 (2016) 379–387, <http://dx.doi.org/10.1016/j.envres.2016.01.017>.
- [24] R. Bhandari, J. Xiao, A. Shankar, Urinary bisphenol A and obesity in US children, *Am. J. Epidemiol.* 177 (2013) 1263–1270, <http://dx.doi.org/10.1093/aje/kws391>.
- [25] D.-K. Li, M. Miao, Z. Zhou, C. Wu, H. Shi, X. Liu, S. Wang, W. Yuan, Urine bisphenol-A level in relation to obesity and overweight in school-age children, *PLoS One* 8 (2013) e65399, <http://dx.doi.org/10.1371/journal.pone.0065399>.
- [26] L.N. Vandenberg, P.A. Hunt, M.J.P. I, F.S. vom Saa, Human exposures to bisphenol A: mismatches between data and assumptions, *Rev. Environ. Health* 28 (2013) 37, <http://dx.doi.org/10.1515/reveh-2012-0034>.
- [27] F.S. vom Saal, W.V. Welshons, Evidence that bisphenol A (BPA) can be accurately measured without contamination in human serum and urine, and that BPA causes numerous hazards from multiple routes of exposure, *Mol. Cell. Endocrinol.* 398 (2014) 101–113, <http://dx.doi.org/10.1016/j.mce.2014.09.028>.
- [28] EFSA, Processing Aids Scientific Opinion on the risks to public health related to the presence of bisphenol A (BPA) in foodstuffs, *EFSA J.* 13 (2015) 3978, <http://dx.doi.org/10.2903/j.efsa.2015.3978>.
- [29] L.N. Vandenberg, M.V. Maffini, C. Sonnenschein, B.S. Rubin, A.M. Soto, Bisphenol-A and the great divide: a review of controversies in the field of endocrine disruption, *Endocr. Rev.* 30 (2009) 75–95, <http://dx.doi.org/10.1210/er.2008-0021>.
- [30] J. Teeguarden, S. Hanson-Drury, J.W. Fisher, D.R. Doerge, Are typical human serum BPA concentrations measurable and sufficient to be estrogenic in the general population? *Food Chem. Toxicol.* 62 (2013) 949–963, <http://dx.doi.org/10.1016/j.fct.2013.08.001>.
- [31] J.G. Hengstler, H. Foth, T. Gebel, P.J. Kramer, W. Lilienblum, H. Schweinfurth, W. Völkel, K.M. Wollin, U. Gundert-Remy, Critical evaluation of key evidence on the human health hazards of exposure to bisphenol A, *Crit. Rev. Toxicol.* 41 (2011) 263–291, <http://dx.doi.org/10.3109/10408444.2011.558487>.
- [32] W. Völkel, Why did researchers not use realistic doses in animal studies of bisphenol A? *Arch. Toxicol.* 91 (2017) 1519–1522, <http://dx.doi.org/10.1007/s00204-016-1840-6>.
- [33] F. Cutanda, H.M. Koch, M. Esteban, J. Sánchez, J. Angerer, A. Castaño, Urinary levels of eight phthalate metabolites and bisphenol A in mother–child pairs from two Spanish locations, *Int. J. Hyg. Environ. Health* 218 (2015) 47–57, <http://dx.doi.org/10.1016/j.ijheh.2014.07.005>.
- [34] A. Covaci, E.D. Hond, T. Geens, E. Govarts, G. Koppen, H. Frederiksen, L.E. Knudsen, T.A. Mørck, A.C. Gutleb, C. Guignard, E. Cocco, M. Horvat, E. Heath, T. Kosjek, D. Mazej, J.S. Tratnik, A. Castaño, M. Esteban, F. Cutanda, J.J. Ramos, M. Berglund, K. Larsson, B.A.G. Jönsson, P. Biot, L. Casteleyn, R. Joas, A. Joas, L. Bloemen, O. Sepai, K. Exley, G. Schoeters, J. Angerer, M. Kolossa-Gehring, U. Fiddicke, D. Aerts, H.M. Koch, Urinary BPA measurements in children and mothers from six European member states: overall results and determinants of exposure, *Environ. Res.* 141 (2015) 77–85, <http://dx.doi.org/10.1016/j.envres.2014.08.008>.
- [35] M. Kasper-Sonnenberg, H.M. Koch, J. Wittsiepe, T. Brüning, M. Wilhelm, Phthalate metabolites and bisphenol A in urines from German school-aged children: results of the Duisburg Birth Cohort and Bochum Cohort Studies, *Int. J. Hyg. Environ. Health* 217 (2014) 830–838, <http://dx.doi.org/10.1016/j.ijheh.2014.06.001>.
- [36] W. Völkel, T. Colnot, G.A. Csanády, J.G. Filser, W. Dekant, Metabolism and kinetics of bisphenol A in humans at low doses following oral administration, *Chem. Res. Toxicol.* 15 (2002) 1281–1287, <http://dx.doi.org/10.1021/tx025548t>.
- [37] W. Völkel, N. Bittner, W. Dekant, Quantitation of bisphenol A and bisphenol A glucuronide in biological samples by high performance liquid chromatography-tandem mass spectrometry, *Drug Metab. Dispos.* 33 (2005) 1748–1757, <http://dx.doi.org/10.1124/dmd.105.005454>.
- [38] W. Dekant, W. Völkel, Human exposure to bisphenol A by biomonitoring: methods, results and assessment of environmental exposures, *Toxicol. Appl. Pharmacol.* 228 (2008) 114–134, <http://dx.doi.org/10.1016/j.taap.2007.12.008>.
- [39] J.G. Teeguarden, N.C. Twaddle, M.I. Churchwell, X. Yang, J.W. Fisher, L.M. Seryak, D.R. Doerge, 24-hour human urine and serum profiles of bisphenol A following ingestion in soup: individual pharmacokinetic data and emographics, *Data in Brief* 4 (2015) 83–86, <http://dx.doi.org/10.1016/j.dib.2015.03.002>.
- [40] J.G. Teeguarden, A.M. Calafat, X. Ye, D.R. Doerge, M.I. Churchwell, R. Gunawan, M.K. Graham, Twenty-four hour human urine and serum profiles of bisphenol A during high-dietary exposure, *Toxicol. Sci.* 123 (2011) 48–57, <http://dx.doi.org/10.1093/toxsci/kfr160>.
- [41] X. Yang, D.R. Doerge, J.G. Teeguarden, J.W. Fisher, Development of a physiologically based pharmacokinetic model for assessment of human exposure to bisphenol A, *Toxicol. Appl. Pharmacol.* 289 (2015) 442–456, <http://dx.doi.org/10.1016/j.taap.2015.10.016>.
- [42] H.M. Koch, A.M. Calafat, Human body burdens of chemicals used in plastic manufacture, *Philos. Trans. R. Soc. Lond. B Biol. Sci.* 364 (2009) 2063–2078, <http://dx.doi.org/10.1098/rstb.2008.0208>.
- [43] A.M. Calafat, M.P. Longnecker, H.M. Koch, S.H. Swan, R. Hauser, L.R. Goldman, Optimal exposure biomarkers for nonpersistent chemicals in environmental epidemiology, *Environ. Health Perspect.* 123 (2015) A166–A168, <http://dx.doi.org/10.1289/ehp.1510041>.
- [44] A.M. Calafat, H.M. Koch, S.H. Swan, R. Hauser, L.R. Goldman, B.P. Lanphear, M.P. Longnecker, R.A. Rudel, S.L. Teitelbaum, R.M. Whyatt, M.S. Wolff, Misuse of blood serum to assess exposure to bisphenol A and phthalates, *Breast Cancer Res.* 15 (2013) 403, <http://dx.doi.org/10.1186/bcr3494>.
- [45] A.G. Asimakopoulou, N.S. Thomaidis, M.A. Koupparis, Recent trends in biomonitoring of bisphenol A, 4-t-octylphenol, and 4-nonylphenol, *Toxicol. Lett.* 210 (2012) 141–154, <http://dx.doi.org/10.1016/j.toxlet.2011.07.032>.
- [46] M.M. Plassmann, W. Brack, M. Krauss, Extending analysis of environmental pollutants in human urine towards screening for suspected compounds, *J. Chromatogr. A* 1394 (2015) 18–25, <http://dx.doi.org/10.1016/j.chroma.2015.03.040>.
- [47] M.A. Fernández-Peralbo, M.D. Luque de Castro, Preparation of urine samples prior to targeted or untargeted metabolomics mass-spectrometry analysis, *Trends Anal. Chem.* 41 (2012) 75–85, <http://dx.doi.org/10.1016/j.trac.2012.08.011>.
- [48] H.M. Koch, M. Kolossa-Gehring, C. Schröter-Kermani, J. Angerer, T. Brüning, Bisphenol A in 24 h urine and plasma samples of the German Environmental Specimen Bank from 1995 to 2009: A retrospective exposure evaluation, *J. Expo. Sci. Environ. Epidemiol.* 22 (2012) 610–616, <http://dx.doi.org/10.1038/jes.2012.39>.
- [49] M. Kasper-Sonnenberg, J. Wittsiepe, H.M. Koch, H. Fromme, M. Wilhelm, Determination of bisphenol A in urine from mother–child pairs—results from the Duisburg birth cohort study, Germany, *J. Toxicol. Environ. Health A* 75 (2012) 429–437, <http://dx.doi.org/10.1080/15287394.2012.674907>.
- [50] S.Y. Lee, N.-H. Park, E.-K. Jeong, J.-W. Wi, C.-J. Kim, J.Y. Kim, M.K. In, J. Hong, Comparison of GC/MS and LC/MS methods for the analysis of propofol and its metabolites in urine, *J. Chromatogr. B* 900 (2012) 1–10, <http://dx.doi.org/10.1016/j.jchromb.2012.05.011>.
- [51] E.R. Perez, J.A. Knapp, C.K. Horn, S.L. Stillman, J.E. Evans, D.P. Arfsten, Comparison of LC–MS–MS and GC–MS analysis of benzodiazepine compounds included in the drug demand reduction urinalysis program, *J. Anal. Toxicol.* 40 (2016) 201–207, <http://dx.doi.org/10.1093/jat/bkv140>.
- [52] T. Aaroe Mørck, Chapter 3G bisphenol A, in: L. Knudsen, F.M. Domenicom (Eds.), *Biomarkers and Human Biomonitoring*, The Royal Society of Chemistry, 2012, pp. 360–380.
- [53] M. Anastassiades, S.J. Lehotay, D. Stajnbaher, F.J. Schenck, Fast and easy multi-residue method employing acetonitrile extraction/partitioning and dispersive solid-phase extraction for the determination of pesticide residues in produce, *J. AOAC Int.* 86 (2003) 412–431.
- [54] A. Wiłkowska, M. Biziuk, Determination of pesticide residues in food matrices using the QuEChERS methodology, *Food Chem.* 125 (2011) 803–812, <http://dx.doi.org/10.1016/j.foodchem.2010.09.094>.
- [55] B. Socas-Rodríguez, J. González-Sálamo, A.V. Herrera-Herrera, J. Hernández-Borges, M.A. Rodríguez-Delgado, Recent Advances and Developments in the QuEChERS Method, *Comprehensive Analytical Chemistry*, Elsevier, 2017, pp. 1–55.
- [56] A. Jakimka, B. Huerta, Z. Bargańska, A. Kot-Wasik, S. Rodríguez-Mozaz, D. Barceló, Development of a liquid chromatography–tandem mass spectrometry procedure for determination of endocrine disrupting compounds in fish from Mediterranean rivers, *J. Chromatogr. A* 1306 (2013) 44–58, <http://dx.doi.org/10.1016/j.chroma.2013.07.050>.
- [57] C. Pouech, M. Tournier, N. Quignot, A. Kiss, L. Wiest, F. Lafay, M.-M. Flament-Waton, E. Lemazurier, C. Cren-Olivé, Multi-residue analysis of free and conjugated hormones and endocrine disruptors in rat testis by QuEChERS-based extraction and LC-MS/MS, *Anal. Bioanal. Chem.* 402 (2012) 2777–2788, <http://dx.doi.org/10.1007/s00216-012-5723-2>.
- [58] J. Dominguez-Alvarez, E. Rodriguez-Gonzalo, J. Hernandez-Mendez, R. Carabias-Martinez, Programed nebulizing-gas pressure mode for quantitative capillary electrophoresis-mass spectrometry analysis of endocrine disruptors in honey, *Electrophoresis* 33 (2012) 2374–2381, <http://dx.doi.org/10.1002/elps.201100577>.
- [59] J.S. Munaretto, G. Ferronato, L.C. Ribeiro, M.L. Martins, M.B. Adaiame, R. Zanella, Development of a multiresidue method for the determination of endocrine disruptors in fish fillet using gas chromatography–triple quadrupole tandem mass spectrometry, *Talanta* 116 (2013) 827–834, <http://dx.doi.org/10.1016/j.talanta.2013.07.047>.
- [60] S.C. Cunha, C. Cunha, A.R. Ferreira, J.O. Fernandes, Determination of bisphenol A and bisphenol B in canned seafood combining QuEChERS extraction with dispersive liquid–liquid microextraction followed by gas chromatography–mass spectrometry, *Anal. Bioanal. Chem.* 404 (2012) 2453–2463, <http://dx.doi.org/10.1007/s00216-012-6389-5>.
- [61] S.C. Cunha, J.O. Fernandes, Assessment of bisphenol A and bisphenol B in canned vegetables and fruits by gas chromatography–mass spectrometry after QuEChERS and dispersive liquid–liquid microextraction, *Food Control* 33 (2013) 549–555, <http://dx.doi.org/10.1016/j.foodcont.2013.03.028>.
- [62] M. Faraji, M. Noorani, B. Nasiri Sahneh, Quick, easy, cheap, effective, rugged, and safe method followed by ionic liquid-dispersive liquid–liquid microextraction for the determination of trace amount of bisphenol A in canned foods, *Food Anal. Methods* 10 (2017) 764–772, <http://dx.doi.org/10.1007/s12161-016-0635-y>.
- [63] S.C. Cunha, C. Oliveira, J.O. Fernandes, Development of QuEChERS-based extraction and liquid chromatography–tandem mass spectrometry method for simultaneous quantification of bisphenol A and tetrabromobisphenol A in seafood: fish, bivalves, and seaweeds, *Anal. Bioanal. Chem.* 409 (2017) 151–160, <http://dx.doi.org/10.1007/s00216-016-9980-3>.
- [64] E. Fasano, T. Cirillo, F. Esposito, S. Lacorte, Migration of monomers and plasticizers from packed foods and heated microwave foods using QuEChERS sample preparation and gas chromatography/mass spectrometry, *Lebensm. Wiss. Technol.* 64 (2015) 1015–1021, <http://dx.doi.org/10.1016/j.lwt.2015.06.066>.
- [65] J. Lapviboonsuk, N. Leepipatiboon, A simple method for the determination of bisphenol A diglycidyl ether and its derivatives in canned fish, *Anal. Methods* 6 (2014) 5666–5672, <http://dx.doi.org/10.1039/C4AY00757C>.
- [66] M. Roca, N. Leon, A. Pastor, V. Yusà, Comprehensive analytical strategy for bio-monitoring of pesticides in urine by liquid chromatography–orbitrap high resolution mass spectrometry, *J. Chromatogr. A* 1374 (2014) 66–76, <http://dx.doi.org/10.1016/j.chroma.2014.11.010>.
- [67] K. Usui, Y. Hayashizaki, T. Minagawa, M. Hashiyada, A. Nakano, M. Funayama, Rapid determination of disulfotol and its oxidative metabolites in human whole

- blood and urine using QuEChERS extraction and liquid chromatography–tandem mass spectrometry, *Leg. Med. (Tokyo)* 14 (2012) 309–316, <http://dx.doi.org/10.1016/j.legalmed.2012.06.005>.
- [68] A. López, P. Dualde, V. Yusà, C. Coscollà, Retrospective analysis of pesticide metabolites in urine using liquid chromatography coupled to high-resolution mass spectrometry, *Talanta* 160 (2016) 547–555, <http://dx.doi.org/10.1016/j.talanta.2016.07.065>.
- [69] J.L. Westland, F.L. Dorman, QuEChERS extraction of benzodiazepines in biological matrices, *J. Pharm. Anal.* 3 (2013) 509–517, <http://dx.doi.org/10.1016/j.jpha.2013.04.004>.
- [70] V. Alves, C. Conceição, J. Gonçalves, H.M. Teixeira, J.S. Câmara, Improved analytical approach based on quEChERS/UHPLC-PDA for quantification of fluoxetine, clomipramine and their active metabolites in human urine samples, *J. Anal. Toxicol.* 41 (2017) 45–53, <http://dx.doi.org/10.1093/jat/bkw077>.
- [71] D.Y. Bang, S.K. Byeon, M.H. Moon, Rapid and simple extraction of lipids from blood plasma and urine for liquid chromatography–tandem mass spectrometry, *J. Chromatogr. A* 1331 (2014) 19–26, <http://dx.doi.org/10.1016/j.chroma.2014.01.024>.
- [72] M. Jaffé, Ueber den Niederschlag, welchen Pikrinsäure in normalem harn erzeugt und über eine neue reaction des kreatinins. (About the precipitation caused by pikrinic acid in normal urine and about a new reaction of creatinine) [in German], *Physiol. Chem.* 10 (1986) 391–400.
- [73] H.-W. Kuo, W.-H. Ding, Trace determination of bisphenol A and phytoestrogens in infant formula powders by gas chromatography–mass spectrometry, *J. Chromatogr. A* 1027 (2004) 67–74, <http://dx.doi.org/10.1016/j.chroma.2003.08.084>.
- [74] ICH, ICH Harmonised Tripartite Guideline, Validation of Analytical Procedures: Text And Methodology, (1996) http://www.ich.org/fileadmin/Public_Web_Site/ICH_Products/Guidelines/Quality/Q2_R1/Step4/Q2_R1_Guideline.pdf DOI 02-01-2016.
- [75] M.M. Moein, A. El Beqqali, M. Abdel-Rehim, Bioanalytical method development and validation: critical concepts and strategies, *J. Chromatogr. B* 1043 (2017) 3–11, <http://dx.doi.org/10.1016/j.jchromb.2016.09.028>.
- [76] I. Taverniers, M. De Loose, E. Van Bockstaele, Trends in quality in the analytical laboratory. II. Analytical method validation and quality assurance, *Trends Anal. Chem.* 23 (2004) 535–552, <http://dx.doi.org/10.1016/j.trac.2004.04.001>.
- [77] K. Wilczewska, J. Namieśnik, A. Wasik, Troubleshooting of the determination of bisphenol A at ultra-trace levels by liquid chromatography and tandem mass spectrometry, *Anal. Bioanal. Chem.* 408 (2016) 1009–1013, <http://dx.doi.org/10.1007/s00216-015-9215-z>.
- [78] D.A. Markham, J.M. Waechter Jr., M. Wimber, N. Rao, P. Connolly, J.C. Chuang, S. Hentges, R.N. Shiotsuka, S. Dimond, A.H. Chappelle, Development of a method for the determination of bisphenol A at trace concentrations in human blood and urine and elucidation of factors influencing method accuracy and sensitivity, *J. Anal. Toxicol.* 34 (2010) 293–303.
- [79] P. Payá, M. Anastassiades, D. Mack, I. Sigalova, B. Tasdelen, J. Oliva, A. Barba, Analysis of pesticide residues using the Quick Easy Cheap Effective Rugged and Safe (QuEChERS) pesticide multiresidue method in combination with gas and liquid chromatography and tandem mass spectrometric detection, *Anal. Bioanal. Chem.* 389 (2007) 1697–1714, <http://dx.doi.org/10.1007/s00216-007-1610-7>.
- [80] Method AOAC, Pesticide residues in foods by acetonitrile extraction and partitioning with magnesium sulphate, *Off. Methods Anal.* 01 (2007) 2007.
- [81] EN 15662, Foods of plant origin- determination of pesticides residues using GC–MS and/or LC–MS/MS following acetonitrile extraction/partitioning and clean-up by dispersive SPE (QuEChERS method), (2007).
- [82] R. Raina-Fulton, New trends in pesticide residue analysis in cereals, nutraceuticals, baby foods, and related processed consumer products, *J. AOAC Int.* 98 (2015) 1163–1170, <http://dx.doi.org/10.5740/jaoacint.SGE2Raina-Fulton>.
- [83] L. Tang, P. Kebarle, Dependence of ion intensity in electrospray mass spectrometry on the concentration of the analytes in the electrosprayed solution, *Anal. Chem.* 65 (1993) 3654–3668, <http://dx.doi.org/10.1021/ac00072a020>.
- [84] P. Panuwet, R.E. Hunter, P.E. D'Souza, X. Chen, S.A. Radford, J.R. Cohen, M.E. Marder, K. Kartavenka, P.B. Ryan, D.B. Barr, Biological matrix effects in quantitative tandem mass spectrometry-based analytical methods: advancing bio-monitoring, *Crit. Rev. Anal. Chem.* 46 (2016) 93–105, <http://dx.doi.org/10.1080/10408347.2014.980775>.
- [85] M.L. Chiu, W. Lawi, S.T. Snyder, P.K. Wong, J.C. Liao, V. Gau, Matrix effects—a challenge toward automation of molecular analysis, *JALA* 15 (2010) 233–242, <http://dx.doi.org/10.1016/j.jala.2010.02.001>.
- [86] S. Uclés, A. Lozano, A. Sosa, P. Parrilla Vázquez, A. Valverde, A.R. Fernández-Alba, Matrix interference evaluation employing GC and LC coupled to triple quadrupole tandem mass spectrometry, *Talanta* 174 (2017) 72–81, <http://dx.doi.org/10.1016/j.talanta.2017.05.068>.
- [87] D.J. Anderson, E.M. Brozek, K.J. Cox, C.A. Porucznik, D.G. Wilkins, Biomonitoring method for bisphenol A in human urine by ultra-high-performance liquid chromatography–tandem mass spectrometry, *J. Chromatogr. B* 953 (2014) 53–61, <http://dx.doi.org/10.1016/j.jchromb.2014.01.039>.
- [88] T.A.V. Brigante, L.F.C. Miranda, I.D. de Souza, V.R. Acquaro Junior, M.E.C. Queiroz, Pipette tip dummy molecularly imprinted solid-phase extraction of Bisphenol A from urine samples and analysis by gas chromatography coupled to mass spectrometry, *J. Chromatogr. B* (2017), <http://dx.doi.org/10.1016/j.jchromb.2017.09.038>.